

AtriClip PRO-V® LAA Exclusion System

INSTRUCTIONS FOR USE

PROV35, PROV40, PROV45, PROV50

MD

CAUTION: Federal law (US) restricts this device to sale by or on the order of a physician.

FIGURE 1

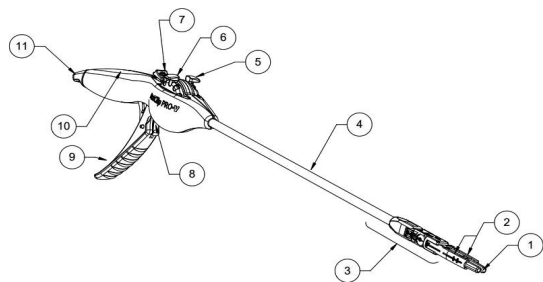


FIGURE 2




FIGURE 3



FIGURE 4




FIGURE 5




FIGURE 6





FIGURE 7



INSTRUCTIONS FOR USE

en

AtriClip PRO-V® LAA Exclusion System

INDICATION FOR USE

The AtriClip LAA Exclusion System is indicated for the exclusion of the heart's left atrial appendage, performed under direct visualization and in conjunction with other cardiac surgical procedures.

Direct visualization, in this context, requires that the surgeon is able to see the heart directly, with or without assistance from a camera, endoscope, etc., or other appropriate viewing technologies.

CONTRAINDICATIONS

1. Do not use this device as a contraceptive tubal occlusion device.
2. Do not use this device if evidence of systemic infection, bacterial endocarditis, or in the presence of infected operating field.

SYSTEM DESCRIPTION

The AtriClip Pro-V LAA Exclusion System contains the V Clip (Clip) for exclusion of the heart's left atrial appendage (LAA). Preclinical animal studies (Kamohara 2005, 2006) demonstrate that complete exclusion with the Clip also results in acute and chronic electrical isolation of the LAA. A human clinical study (Stark 2012) has demonstrated acute electrical isolation. Chronic electrical isolation has not been evaluated in human clinical studies.

The AtriClip Pro-V LAA Exclusion System is a delivery and deployment device preloaded with a V Clip. The V Clip is pre-loaded on a disposable Clip applicator. The V Clip is a permanent implant; device lifetime is equal to patient lifetime. The Clip was determined to be "MR Conditional" per the requirements of standard ASTM F2503-23e1.

The AtriClip Pro-V LAA Exclusion System is used to deliver a preloaded Clip to the target LAA site. The Clip is a sterile, permanent implant composed of Grade 5 Titanium and covered in a knit-braided Polyethylene Terephthalate fabric that contains a small fraction of titanium dioxide. The Pro-V LAA Exclusion System with preloaded V Clip is not made with natural rubber latex and does not contain phthalates. Detailed materials information for implanted V Clip sizes 35 mm to 50 mm are below:

| Material | Mass (g) | CAS # |
|----------------------------|--------------|---|
| Titanium Grade 5 | 2.41 to 3.73 | Titanium, 7440-32-6 Aluminum, 7429-90-5 Vanadium, 7440-62-2 |
| Polyethylene Terephthalate | 0.25 to 0.31 | 25038-59-9 |
| Titanium Dioxide | 0.001 | 13463-67-7 |

ENVIRONMENTAL SPECIFICATIONS

| Storage | Transit |
|--|--|
| Temperature: -29°C / -20°F to 60°C / 140°F | Temperature: -29°C / -20°F to 60°C / 140°F |
| Relative Humidity: 15% to 85% | Relative Humidity: 30% to 85% |
| Atmospheric Pressure: N/A | Atmospheric Pressure: N/A |

PACKAGE CONTENTS

1. One (1) AtriClip LAA Exclusion System
2. One (1) Implant Card and (1) Implant Card Leaflet

The AtriClip Pro-V LAA Exclusion System is supplied STERILE and NON-PYROGENIC in unopened, undamaged package. For single use only. Do not re-sterilize. Do not re-use.

SYSTEM ACCESSORIES

Other devices, not included with the System, may be used in conjunction with the AtriClip Pro-V LAA Exclusion System. These may include but are not limited to the following:

- Selection Guide (CGG100) (Guide)—Packaged Separately
- Minimum 12 mm port

ATRICLIP PRO-V LAA EXCLUSION SYSTEM

NOMENCLATURE (SEE FIGURE 1)

- | | |
|-----------------------------|---------------------------|
| [1] V Clip | [7] Articulation Lock |
| [2] Clip Opening Jaws | [8] Lever Release Trigger |
| [3] End Effector | [9] Activation Lever |
| [4] Shaft | [10] Handle |
| [5] Left/Right Articulation | [11] Deployment Tab |
| [6] Up/Down Articulation | |

⚠ WARNINGS ⚠

Read all instructions carefully for the AtriClip LAA Exclusion System before use and use the device only as intended. Use of the AtriClip LAA Exclusion System should be limited to properly trained and qualified medical personnel. Improper use of this system may lead to device malfunction, failure to provide intended therapy, and/or serious injury to user or patient.

Do not use on tissue which, in the opinion of the surgeon, would not be able to tolerate conventional suture materials or conventional closure techniques (such as surgical stapling). Doing so may result in: tissue trauma, dehiscence, tissue tearing, displacement, and/or lack of desired hemostasis.

The safety and effectiveness of this device in atrial rhythm control management, either alone or in combination with ablative treatment, has not been established.

AtriClip placement that allows blood flow into the LAA may not result in complete exclusion and/or electrical isolation.

DO NOT RESTERILIZE. The AtriClip LAA Exclusion System is provided STERILE and is intended for SINGLE use only. Re-sterilization may cause loss of function or injury to patient.

Evaluate if thrombus is present in LAA. Management of thrombus is dependent on surgeon's standard of care. It is not recommended to place Clip on LAA if there is evidence of thrombus in LAA. Doing so may result in serious patient injury.

COMPLICATIONS

Potential complications associated with the use of the AtriClip Pro-V LAA Exclusion System and procedure include, but are not limited to, those listed below:

- Air embolism
- Allergic reaction to anesthesia, anticoagulant, implant material
- Anaphylactic shock
- Anesthesia risks
- Aneurysm
- Angina
- Arrhythmia needing medical treatment (new onset)
- Arterial or venous dissection and/or perforation
- Arterial rupture
- Arterial spasm
- Arteriovenous fistula
- Atelectasis (major lung collapse with significant symptoms such as cyanosis, extreme shortness of breath, dyspnea, and/or stabbing pain on the affected side)
- Extension of cardiopulmonary/extracorporeal bypass
- Fever
- Gastric motility disorders
- Gastro-intestinal bleed
- Hematoma
- Hematuria
- Hemothorax
- Hypertension
- Hypotension
- Iatrogenic atrial flutter
- Iatrogenic lung injury (e.g., chest tube placement)
- Ischemia
- Kinking of coronary artery
- LAA dehiscence
- LAA tears

- Atrial rupture
- Atrio-esophageal fistula
- AV block requiring permanent pacemaker (new onset)
- Bleeding requiring intervention
- Blood vessel damage
- Cardiac perforation
- Cardiac tamponade
- Cardiac valve injury
- Cerebrovascular accident (CVA)/Transient Ischemic Attack (TIA)/stroke (ischemic or hemorrhagic)
- Chest pain/discomfort
- Compression of coronary artery
- Conduction disturbances
- Congestive heart failure (new onset or exacerbation)
- Coronary artery injury
- Death
- Device breakage/inability to remove
- Device-related death
- Diaphragmatic paralysis (unilateral or bilateral)
- Drug reaction (significant reaction to any procedure related medications requiring treatment, including allergic reaction and anaphylactic shock)
- Emergency during procedure requiring a change in planned access
- Empyema
- Endocarditis (bacterial)
- Esophageal injury
- Esophageal rupture
- Left atrial embolism
- Myocardial infarction (MI)
- Nerve injury (phrenic, laryngeal, thoracic, etc.)
- Pain/discomfort
- Pericardial effusion
- Pericarditis
- Permanent pacemaker
- Persistent chest pain (post discharge surgical incision pain, not angina)
- Phrenic nerve paralysis
- Pleural effusion
- Pneumonia
- Pneumothorax
- Postoperative embolic complications
- Pseudoaneurysm
- Pulmonary edema
- Pulmonary embolism
- Renal insufficiency or failure
- Respiratory distress or failure (breathing problems)
- Sepsis
- Stenosis of left circumflex artery
- Sterility-related infection
- Superficial wound infection
- Surgical site infection
- Systemic adverse reaction due to device corrosion
- Thrombus and/or thromboembolism (including deep vein thrombosis)
- Tissue injury
- Tissue perforation
- Tracheal esophageal trauma
- Vascular access complications

INSTRUCTIONS FOR USE

Surgeon judgment, with the assistance of the Guide, should determine what size Clip to apply.

This IFU is designed to assist in using this product. It is not a reference to surgical techniques.

CLIP SELECTION

⚠ WARNING ⚠

Carefully consider any presurgical treatment the patient may have undergone when selecting Clip size. Preoperative radiotherapy may result in changes to tissue. These changes may, for example, cause the tissue thickness to exceed the indicated range for the selected Clip size. Failure to correctly size the Clip may result in: tissue trauma, dehiscence, tissue tearing, displacement, lack of desired hemostasis, and/or incomplete exclusion of the structure.

1. Using the Guide, determine correct selection of the V Clip (See Figure 2). Clip sizes are located on the device package.

| Labeled Clip Size | LAA Size Range |
|-------------------|-----------------------------|
| 35 mm | 29 – 35 mm (1.14 – 1.38 in) |
| 40 mm | 34 – 40 mm (1.34 – 1.57 in) |
| 45 mm | 39 – 45 mm (1.54 – 1.77 in) |
| 50 mm | 44 – 50 mm (1.73 – 1.97 in) |

⚠️ WARNINGS ⚠️

Do not use on a LAA less than 29 mm (1.14 in) in width and 1 mm (0.04 in) wall thickness. Doing so may result in: tissue trauma, dehiscence, tissue tearing, displacement, and/or lack of desired hemostasis.

Do not use on a LAA greater than 50 mm (1.97 in) when tissue is uncompressed. Doing so may result in incomplete exclusion of the structure.

- Using sterile technique, remove the AtriClip PRO-V LAA Exclusion System from its packaging.

⚠️ WARNINGS ⚠️

If the sterile package is damaged and/or the sterile barrier is breached, discard device and DO NOT USE to avoid the risk of patient infection.

Visually check for rust on the Applier jaws prior to use. The Applier should not be used for durations longer than 1 hour to prevent the formation of rust. Failure to do so may result in a systemic adverse reaction.

⚠️ CAUTION: Do not drop the device as this may induce damage to the device. If the device is dropped, do not use. Replace with a new device.

- Using the Activation Lever on the handle, gently open and close the Clip to assure proper function.

ARTICULATION OF END EFFECTOR

⚠️ CAUTION: Do not attempt to articulate the End Effector while in the locked position. Force applied while in the locked position may cause damage to the device.

- By pushing down and pulling the Articulation Lock backwards (proximal), the End Effector of the AtriClip LAA Exclusion System may be manually articulated up and down and side-to-side by either the articulation levers or pressing on the end effector. The Clip and End Effector can articulate 30° left or right and 60° up or down to take into account anatomical variations in the patient's anatomy (See Figure 3).
- To lock the End Effector in position, press the Articulation Lock forward.

CLIP POSITIONING

⚠️ WARNING ⚠️

Position and deploy Clip in a manner that provides direct visualization of all tissues being accessed. Direct visualization, in this context, requires that the surgeon is able to see the heart directly, with or without assistance from a camera, endoscope, etc., or other appropriate viewing technologies. Poor visualization may result in suboptimal placement and damage or obstruction of surrounding structures.

⚠️ CAUTION: Do not kink or bend the Shaft as this may affect device performance.

- With the Clip in the closed position, maneuver the AtriClip LAA Exclusion System into the targeted dissection plane.
- Gently open the Clip by squeezing the Activation Lever (See Figure 4).

NOTE: The Clip automatically locks in the fully open position by means of a Locking Trigger on the handle of the device. The lock can be disengaged by pressing the Lever Release Trigger.

- Gently position the Clip at the base of the LAA (See Figure 5).
- Position the Clip in a manner that provides clear visualization of all tissues being accessed.
- While the Clip is still affixed to the Deployment Device, ensure that no surrounding structures interfere with or are damaged by the Clip, and that the Clip is placed correctly.
- After the Clip is positioned correctly, grasp the Activation Lever and depress the Lever Release Trigger and slowly release the Activation Lever allowing the Clip to close.

DEPLOYMENT

⚠️ WARNINGS ⚠️

Carefully evaluate Clip position, tissue thickness, and tissue width prior to Clip deployment. To determine appropriate Clip size, refer to the Guide Instructions for Use. Failure to correctly size or deploy the Clip may result in: tissue trauma, dehiscence, tissue tearing, displacement, and/or lack of desired hemostasis.

Unless medically necessary, do not attempt to reposition or remove the Clip after deployment. This may result in tissue damage or tearing.

- If the Clip is not placed correctly, gently open the Clip and reposition as needed.
- Deploy the Clip by slowly pulling the Deployment Tab at the proximal end of the Handle.

NOTE: The Deployment Tab with steel cables may be completely removed from the end of the Handle (See Figure 6).

⚠️ CAUTION: Take care to minimize manipulation of the LAA and Clip after Clip deployment.

- Unlock the End Effector and carefully remove it from the LAA, leaving the Clip and attachment suture behind (See Figure 7).

NOTE: After pulling the Deployment Tab, the AtriClip LAA Exclusion System cannot be used to reposition or remove the Clip.

DISPOSAL INFORMATION

After use, this device should be treated as medical waste and disposed of following hospital protocol.

SERIOUS INCIDENT

Any serious incident that has occurred in relation to this device should be reported to AtriCure.

RETURN OF USED PRODUCT

If, for any reason, this product must be returned to AtriCure, Inc., a return goods authorization (RGA) number is required from AtriCure, Inc., prior to shipping.

If the product has been in contact with blood or body fluids, it must be thoroughly cleaned and disinfected before packing. It should be shipped in either the original carton or an equivalent carton, to prevent damage during shipment; and it should be properly labeled with an RGA number and an indication of the biohazardous nature of the contents of shipment.

Instructions for cleaning and materials, including appropriate shipping containers, proper labeling, and an RGA number may be obtained from AtriCure, Inc.

DISCLAIMER STATEMENTS

Users assume responsibility for approving the acceptable condition of this product before it is used, and for ensuring that the product is only used in the manner described in these instructions for use, including, but not limited to, ensuring that the product is not re-used.

Under no circumstances will AtriCure, Inc. be responsible for any incidental, special or consequential loss, damage, or expense, which is the result of the deliberate misuse or re-use of this product, including any loss, damage, or expense which is related to personal injury or damage to property.

HANDLING INFORMATION: V CLIP

MRI SAFETY INFORMATION



The V Clip is MR Conditional. A patient with the V Clip may be safely scanned under the following conditions. Failure to follow these conditions may result in injury to the patient:

- Nominal Values of Static Magnetic Field:** 1.5-Tesla or 3.0-Tesla
- Maximum Spatial Field Gradient:** 40-T/m (4,000-gauss/cm)
- Type of RF Excitation:** Circularly Polarized (CP) (i.e., Quadrature Transmission)
- Transmit RF Coil Information:** There are no transmit RF coil restrictions
- Operating Mode of MR System:** Normal Operating Mode
- Maximum Whole Body Averaged SAR:** 2-W/kg (Normal Operating Mode)
- Limits on Scan Duration:** Whole body averaged SAR of 2-W/kg for 60 minutes of continuous RF exposure (i.e., per pulse sequence or back-to-back sequences/series without breaks)
- MR Image Artifact:** The presence of this implant produces an imaging artifact. Therefore, carefully select pulse sequence parameters if the implant is located in the area of interest

SYMBOLS GLOSSARY

Refer to the outer package label to see which symbols apply to this product.

| | | | |
|--|---|--|--|
| | Single sterile barrier system with protective packaging outside | | Single sterile barrier system with protective packaging inside |
| | Manufacturer | | Caution |
| | Does not contain phthalates | | Non-pyrogenic |
| | Do not use if package is damaged | | Keep dry |
| | Sterilized using irradiation | | Consult Instructions For Use |
| | Do not re-use | | Do not re-sterilize |
| | Not Made with natural Rubber Latex | | Catalogue Number |
| | Model Number | | Unique Device Identifier |
| | Lot Number | | Use-by date |
| | Prescription Use Only | | MR Conditional |
| | Country of Manufacture | | Medical Device |
| | Transit Temperature limit | | Transit Humidity limit |

REFERENCES

- Kamohara K, et al. A novel device for left atrial appendage exclusion. J Thorac Cardiovasc Surg 2005
- Kamohara K, Fukamachi et al. Evaluation of a novel device for left atrial appendage exclusion: the second-generation atrial exclusion device. J Thorac Cardiovasc Surg 2006
- Starck C, et al. Epicardial left atrial appendage clip occlusion also provides the electrical isolation of the left atrial appendage. Interactive CardioVascular and Thoracic Surgery 15 (2012)

