

AtriClip® FLEX•V® Device

AtriCure



AtriClip Device Performance
with a Clip Deployment Trigger

Enhanced LAA Visualization

One-Handed Application • Suture-Less Clip Deployment

Small Footprint to Minimize the Interference with Adjacent Structures


The AtriClip FLEX•V Device Applies Continual Force
to the Base of the LAA as it Atrophies

Open-Ended
AtriClip

Tip-First
Closure

Continual Force
Applied to the
Base of the LAA



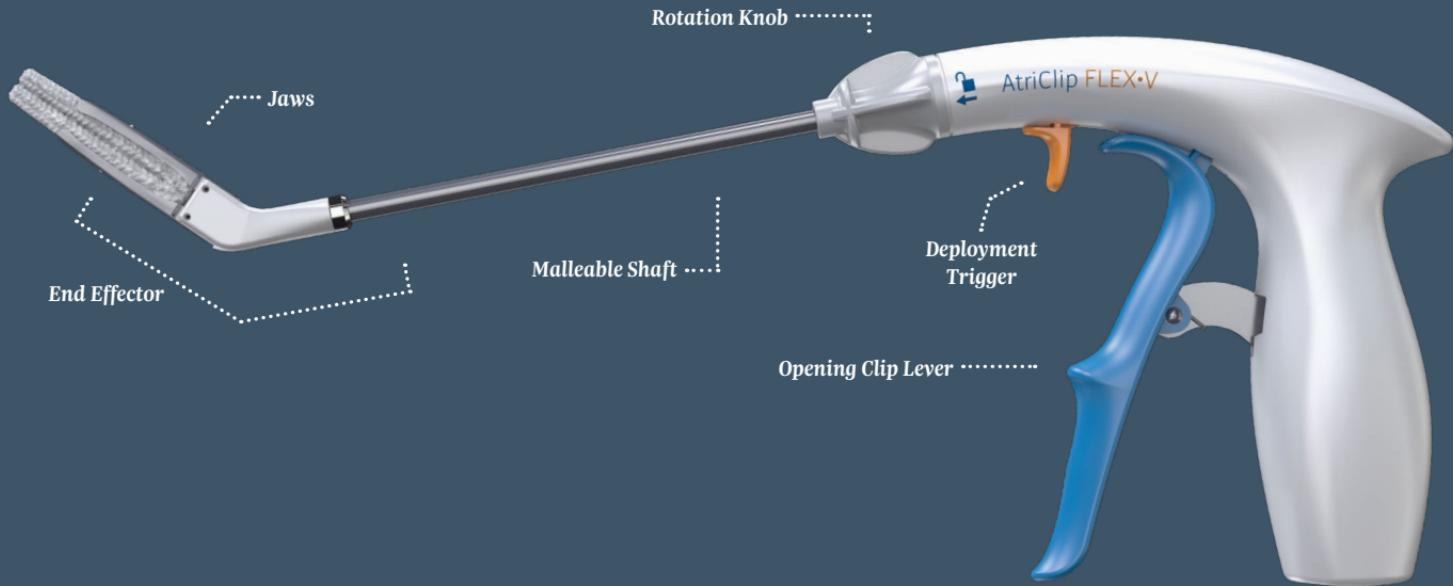

U.S. Indications: The AtriClip LAA Exclusion System is indicated for the exclusion of the heart's left atrial appendage, performed under direct visualization¹, in conjunction with other cardiac surgical procedures.

¹Direct visualization, in this context, requires that the surgeon is able to see the heart directly, with or without assistance from a camera, endoscope, etc., or other appropriate viewing technologies.

Please review the Instructions for Use for a complete listing of contraindications, warnings, precautions and potential adverse events prior to using these devices.

Rx Only.

PM-US-0107D-1127-G

AtriCure